


μQUANT CORE FACILITY (IHV)

CIBR: Center for Innovative Biomedical Resources

CORE INSTRUMENTATION

SPECTRAMAX M2 6-96 WELL PLATE READER

- 6-well to 96-well plate reading capability
- Built-in absorbance and fluorescence
- Absorbance wavelength between 200 nm and 1000 nm, excitation wavelength between 250 nm and 850 nm, and emission wavelength between 360 nm and 850 nm



WALLAC VICTOR 2 MULTI-ANALYTE PLATE READER

- Complete platform for quantitative detection of light-emitting or light absorbing markers
- Luminescence, fluorescence, time-resolved fluorescence (DELFI), and photometer



VERITAS MICROPLATE LUMINOMETER

- Read glow and flash luminescent reactions in 96-well plates

BIO-PLEX 200 SYSTEM

- Simultaneously quantitate up to 100 analytes per sample from culture media and serum
- Automatically analyze up to 96 samples in 30 min
- Instantly customize your assay by mixing Bio-Plex assay, or create your own assays
- Dramatically increase the amount of useful data obtained from a single sample



StepOnePlus REAL-TIME PCR SYSTEM

- 96-well Real-Time PCR instrument with sensitive 4-color optical LED recording system

SimpliAmp PCR THERMAL CYCLER

MISSION

The μQUANT Core Facility housed within the Institute of Human Virology provides quality immunological analyses of biological analytes to researchers at the UM SOM, as well as other collaborators locally and nationally. Our aim is to provide consistent service that allows researchers to compare results generated this week with those gathered last month or a year ago.

CORE SERVICES

Services offered include, but are not limited to:

- ELISAs
- PBMCs
- Immunoassay setup & protocol establishment
- Luminex assays
- Mycoplasma & endotoxin testing
- Monoclonal antibody and recombinant protein screening, production, purification, & labeling
- HIV, SIV, & SHIV culture
- TCID50 and neutralization assays
- Quantitative PCR

μQUANT CORE FACILITY (IHV)

CIBR: Center for Innovative Biomedical Resources

SpectroMax M2 Data

		PLATE 2											
		1	2	3	4	5	6	7	8	9	10	11	12
A	2.200	2.147	1.874	1.912	1.744	1.862	2.060	1.978	1.777	2.375	-0.023	-0.023	
B	1.393	1.337	1.923	1.563	1.889	1.534	2.081	1.830	2.045	2.311	-0.023	-0.023	
C	0.831	0.816	1.341	1.165	1.158	1.630	1.241	0.987	0.995	2.074	-0.023	-0.023	
D	0.447	0.407	0.905	1.016	0.802	1.686	0.703	0.812	0.935	2.207	-0.023	-0.023	
E	0.252	0.221	2.003	2.224	2.313	1.133	2.277	2.399	2.393	1.924	-0.023	-0.023	
F	0.137	0.092	1.608	2.040	1.505	1.595	1.757	1.944	1.993	2.110	-0.023	-0.022	
G	0.071	0.071	1.004	0.528	1.092	0.020	0.575	0.739	0.706	0.002	-0.023	-0.023	
H	0.003	-0.004	2.074	1.849	1.689	-0.001	1.944	2.080	2.155	0.019	-0.023	-0.023	

Settings Information

Endpoint
 Absorbance
 Lm1 450
 Lm2 570
 More Settings
 Shake Once
 Calibrate On
 Column Priority

CONTACT



Ping-Hsin Rex Lin, MS
 Research Assistant, Laboratory
 plin@ihv.umaryland.edu

LOCATION

Lab: S-632/633, Office: N-562
 Institute of Human Virology (IHV)
 725 West Lombard Street
 Baltimore, MD 21201

410-706-4648
 Fax 410-706-4694



Web Page

<http://ihv.org/research/facility.html>

qPCR Data

PCR Quantification Data

PCR Amp/Cycle Chart

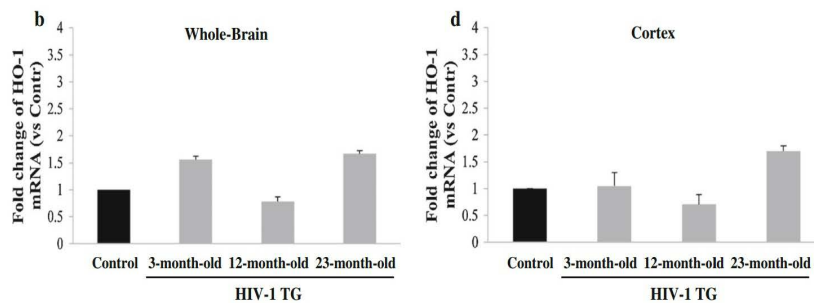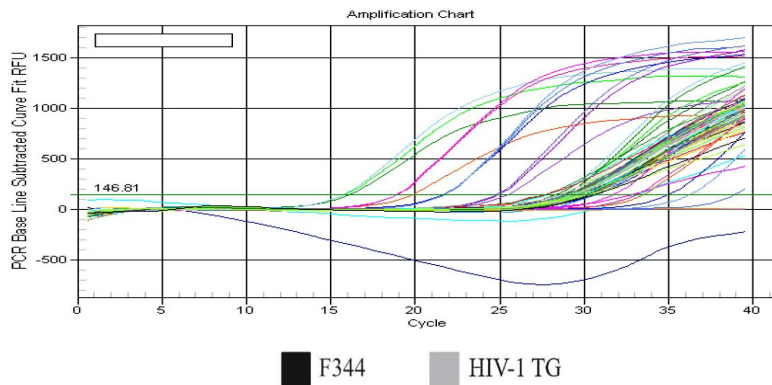

Davinelli S. (2014). Altered expression pattern of Nrf2/HO-1 axis during accelerated-senescence in HIV-1 transgenic rat. *Biogerontology*, 15(5), 449-61